


FIG. 3A


Imaging Plate Insertion

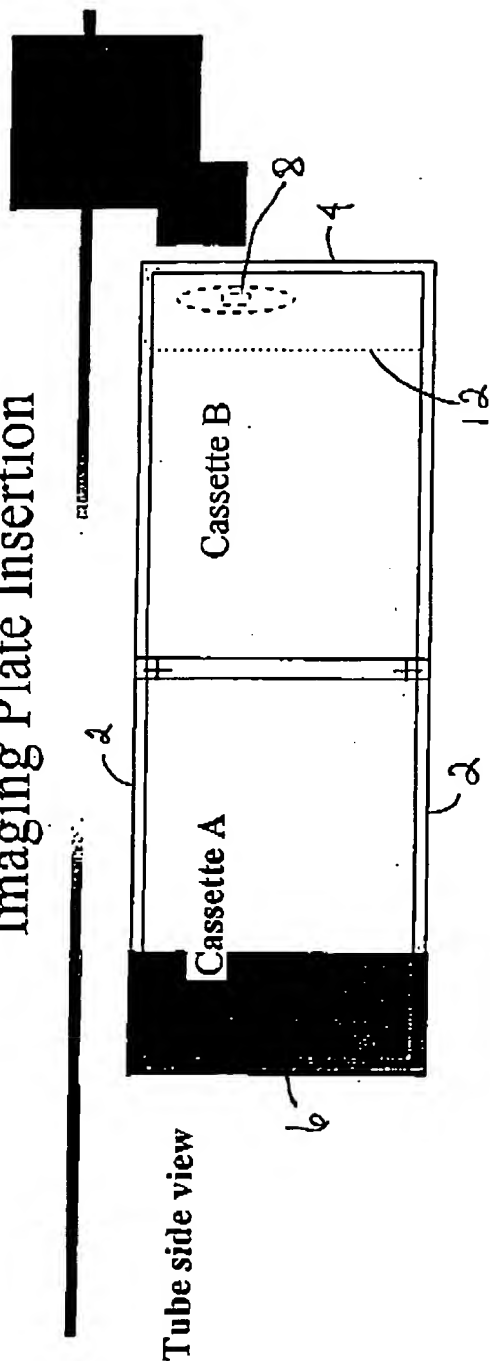

2 Imaging Plates (IP's) are inserted into cassette and overlap slightly

FIG. 3B

Cassette edge view
(Magnified)

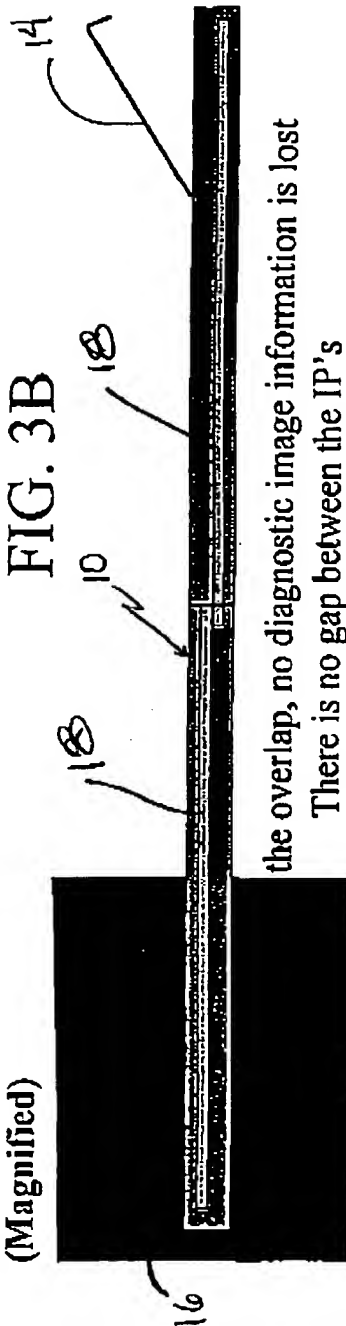

the overlap, no diagnostic image information is lost
There is no gap between the IP's

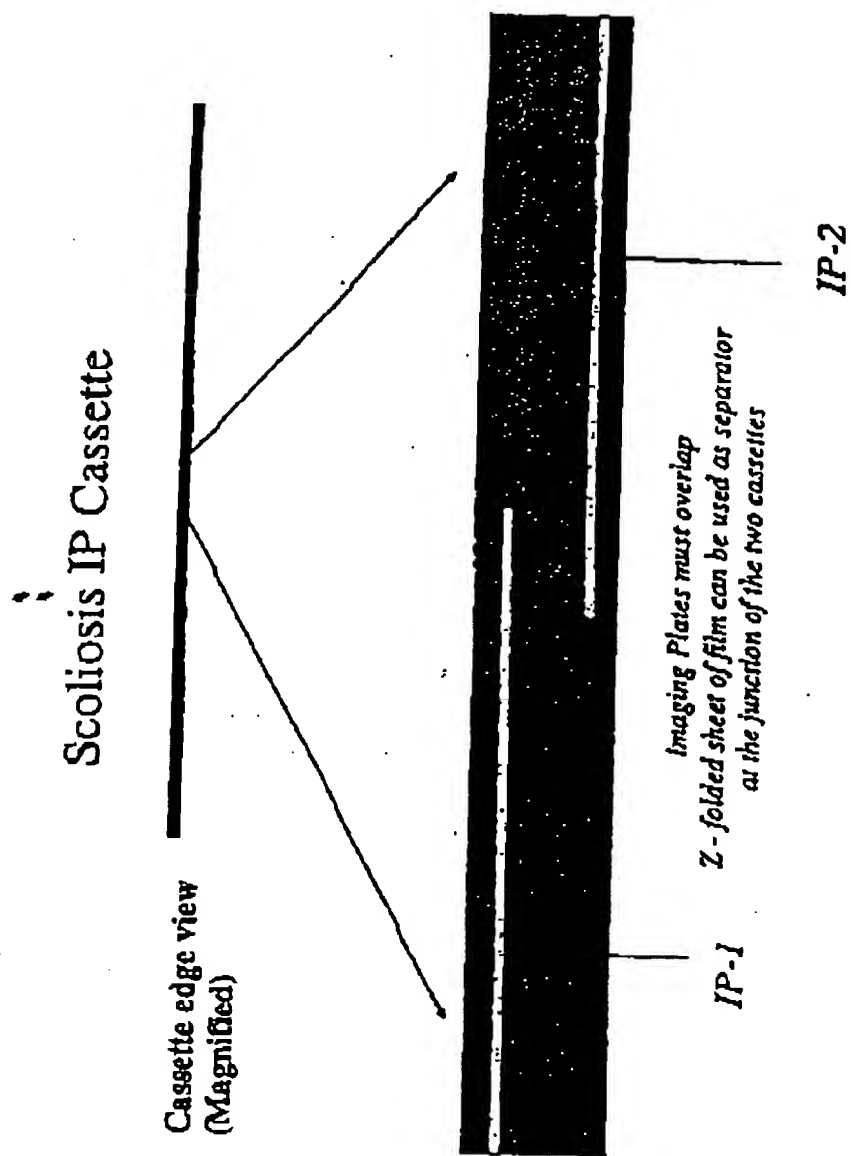


FIG. 5